


OXYTOCIN 2MG



High Performance Liquid Chromatography (HPLC) - Purity Test

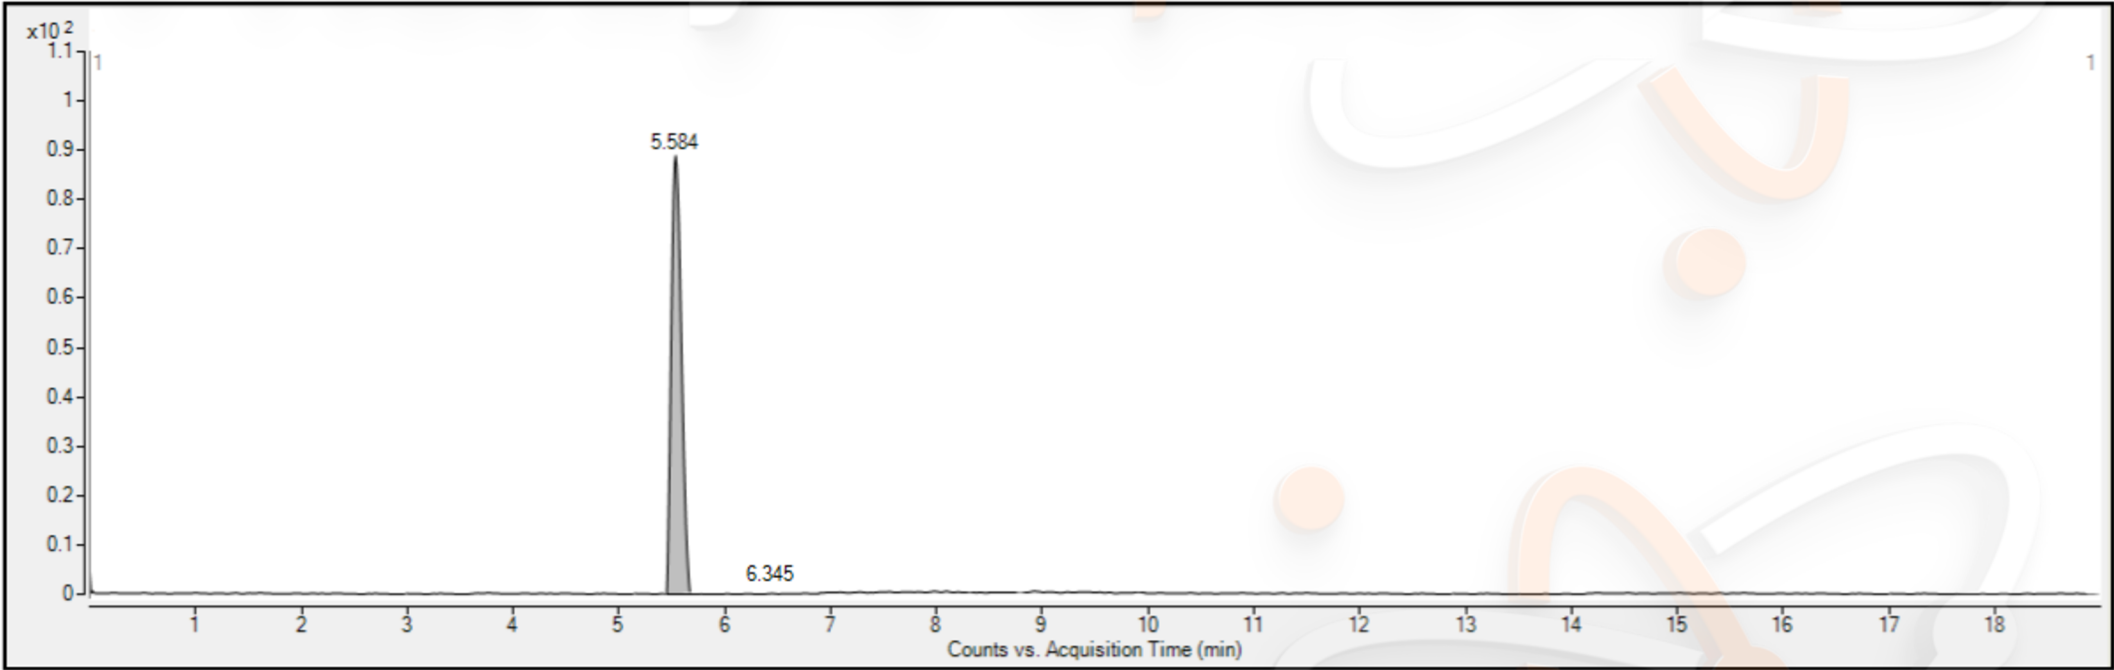

Chromatogram Peaks			
Peak.	RT.	%	Item.
1.	5.984		OXYTOCIN
2.	6.345		

Number of detected peaks: 1

Purity: 99.07
Compound: OXYTOCIN
Analysis date: 8/8/25
Method: HPLC & LCMS Mass Spectrometry
Purity Measured using High Performance Liquid Chromatography
Molecular weight confirmed - 1007.0
Quantity: 2.10 mg per vial

Mass Spectrometry Identify Test



Analysis preformed by:
Richard Sylvester MD

DR Richard Sylvester

PRI-OXYT-00001